

Image-guided therapy and medical robotics tutorial using a LEGO Mindstorms NXT robot and 3D Slicer

Part II: The Basic Tutorial



Danielle F. Pace, B.CmpH

Ron Kikinis, M.D.

Nobuhiko Hata, Ph.D

**Surgical Planning Laboratory,
Brigham and Women's Hospital and
Harvard Medical School**

Funding Information

This tutorial was made possible by grant numbers 5U41RR019703, 5P01CA067165 and 5U54EB005149 from the National Institutes of Health (NIH). Its contents are solely the responsibility of the authors and do not necessarily represent the official views of the NIH. This tutorial was also in part supported by National Science Foundation (NSF) grant number 9731748 and the Center for Integration of Medicine and Innovative Technology (CIMIT).

Goals of the image-guided therapy and medical robotics tutorial

- To demonstrate the typical steps of an image-guided therapy (IGT) or medical robotics procedure.
- To learn in a hands-on manner using a LEGO Mindstorms NXT, a LEGO phantom and sophisticated medical image processing and IGT software (3D Slicer).

The example procedure that we will use to do this is a needle biopsy.


Goals of the basic tutorial

- To learn about the following steps in IGT and medical robotics in a hands-on manner:
 - ✓ Imaging
 - ✓ Preoperative planning
 - ✓ Targeting and tracking
 - ✓ Navigation

The basic tutorial

In the basic tutorial, the phantom is placed in a predefined position relative to the LEGO robot.

Since the relationship between the phantom and the LEGO robot is known, we can use a predefined registration matrix to transform image coordinates into patient (robot) coordinates.

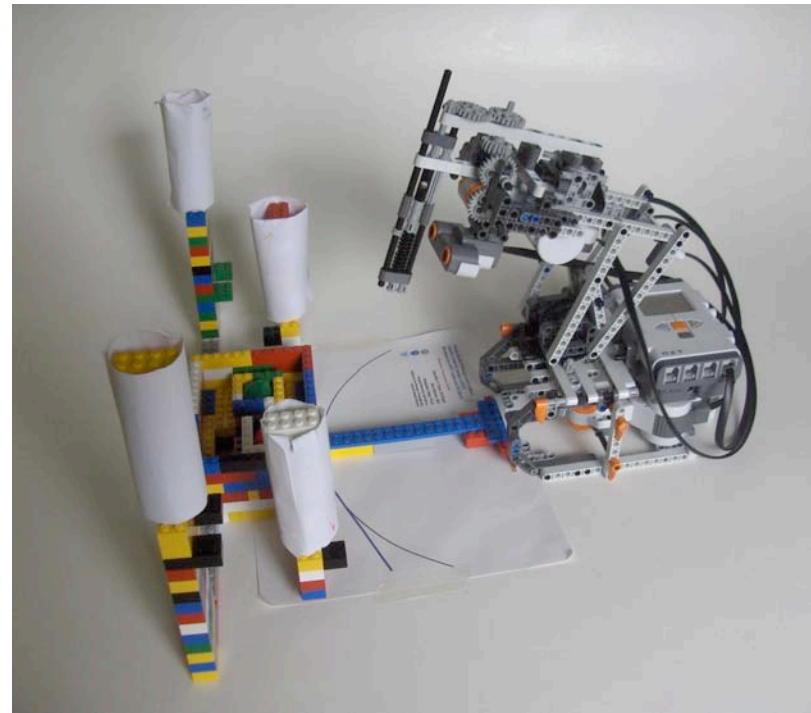


We do not have to perform registration because it has been done already.

Set up the LEGO robot and the phantom

The final
setup:


Instructions
to follow
are in
yellow boxes

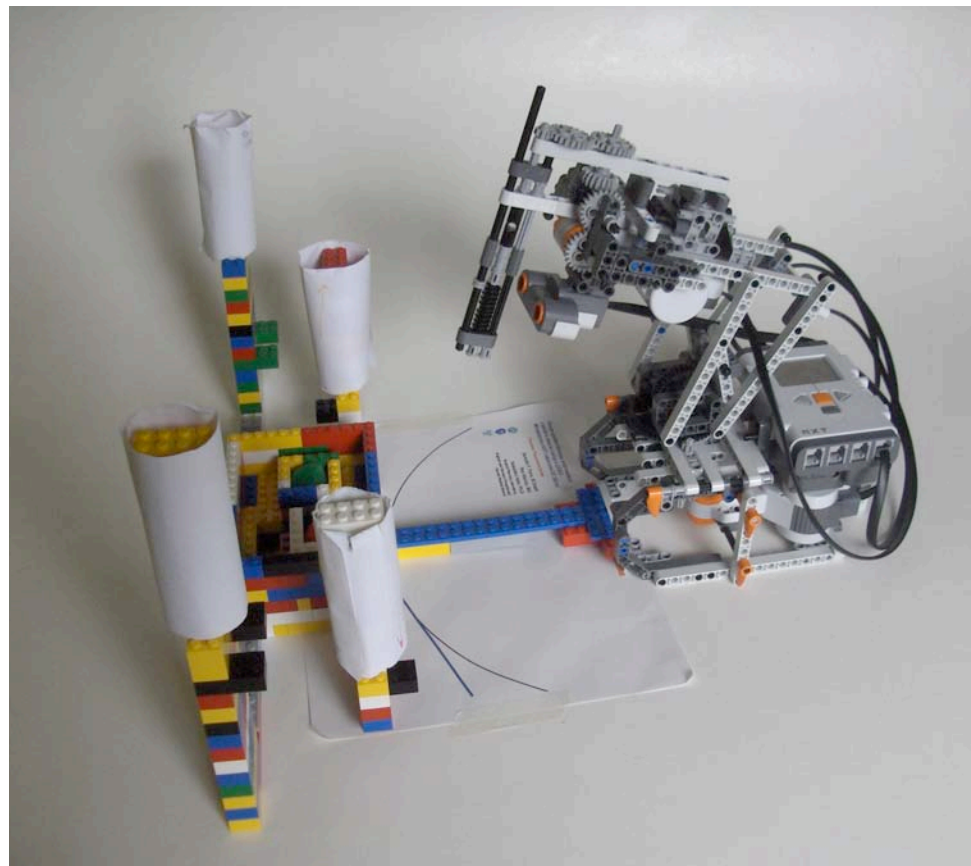

Set up the LEGO robot and the phantom, continued




- Tape the phantom placement guide on a table
- Ensure that there is no wall or other object within a four foot radius around the robot, as walls or other objects will interfere with the ultrasonic sensor used in the advanced tutorial
- Remember that you need to use new batteries or a freshly charged battery pack on the robot.

Set up the LEGO robot and the phantom, continued

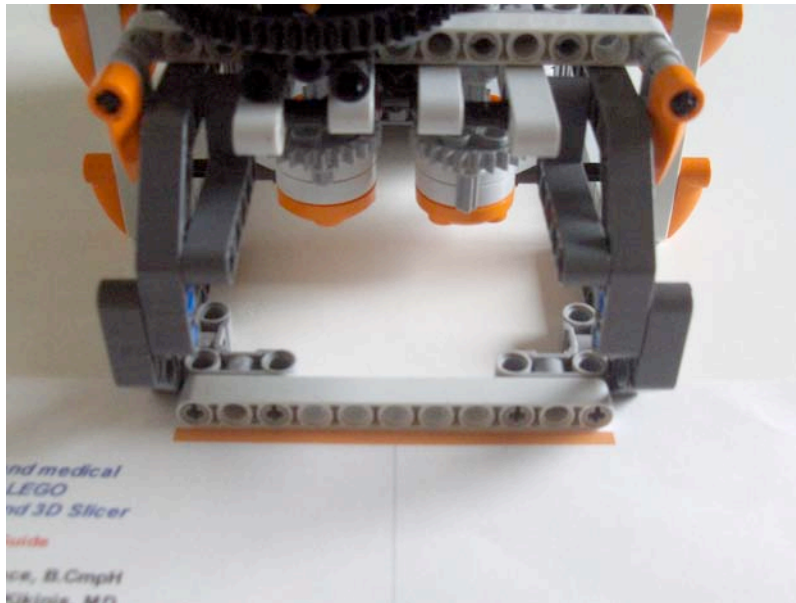

- Position the LEGO robot so that the front piece of the base lines up with the orange line of the phantom placement guide

Set up the LEGO robot and the phantom, continued

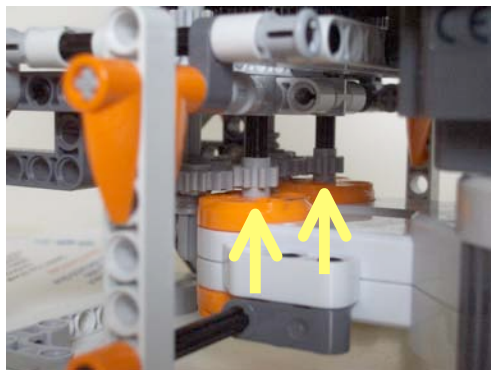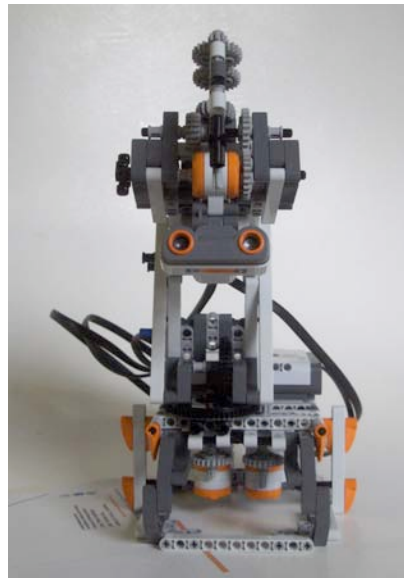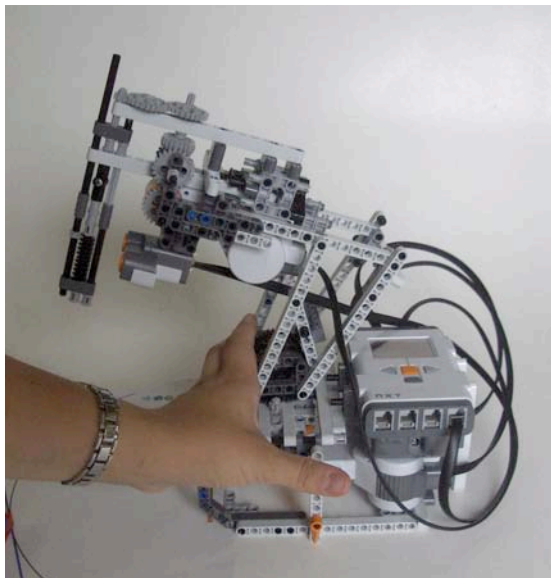

- Position the robot in the “initial position”:
 - robotic arm is pushed all the way back
 - robotic arm is centered
- To move the robotic arm:
 - push the small gears at the back of the robot’s base **up**
 - Freely move the robotic arm into position
 - Push the small gears at the back of the robot’s base back **down** so that they catch on the larger gears


Set up the LEGO robot and the phantom, continued



- Using the gear on the upper right side of the robotic arm, adjust the needle so that it is at its highest possible position while still remaining on the thread.


Set up the LEGO robot and the phantom, continued

- Position the phantom so that the bottom spacer is centered on the front piece of the robot's base.

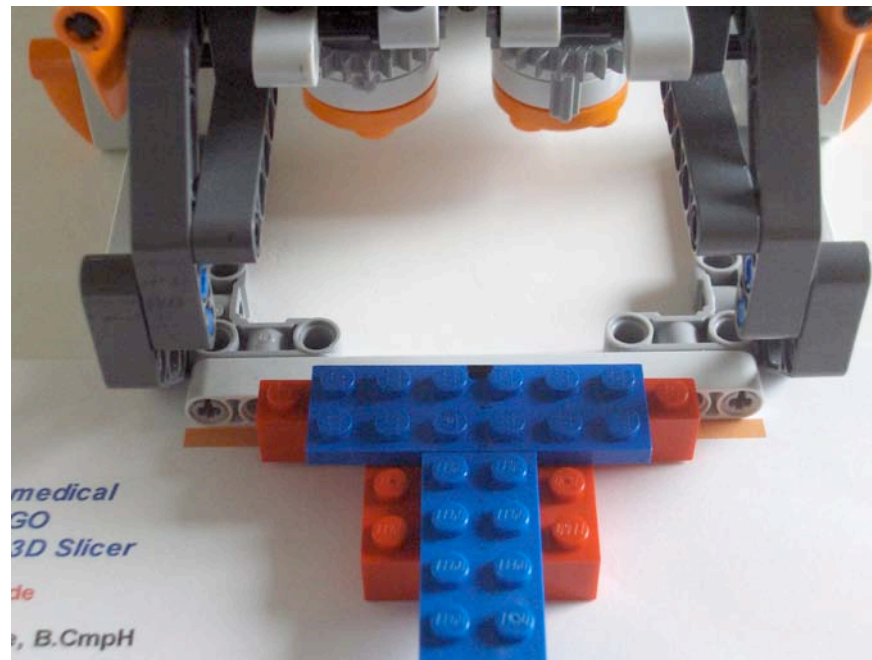


Set up the LEGO robot and the phantom, continued

Your setup should look like this:

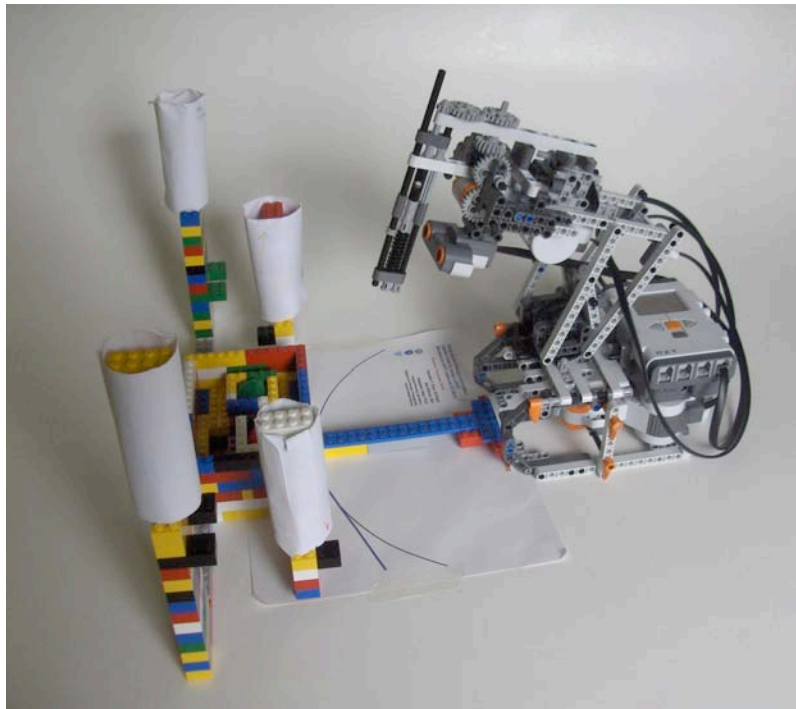

- Connect the robot to the Linux computer using the USB cable provided in the LEGO Mindstorms NXT kit
- Turn the LEGO robot on by pressing the orange button on the NXT brick.

1) Open 3D Slicer

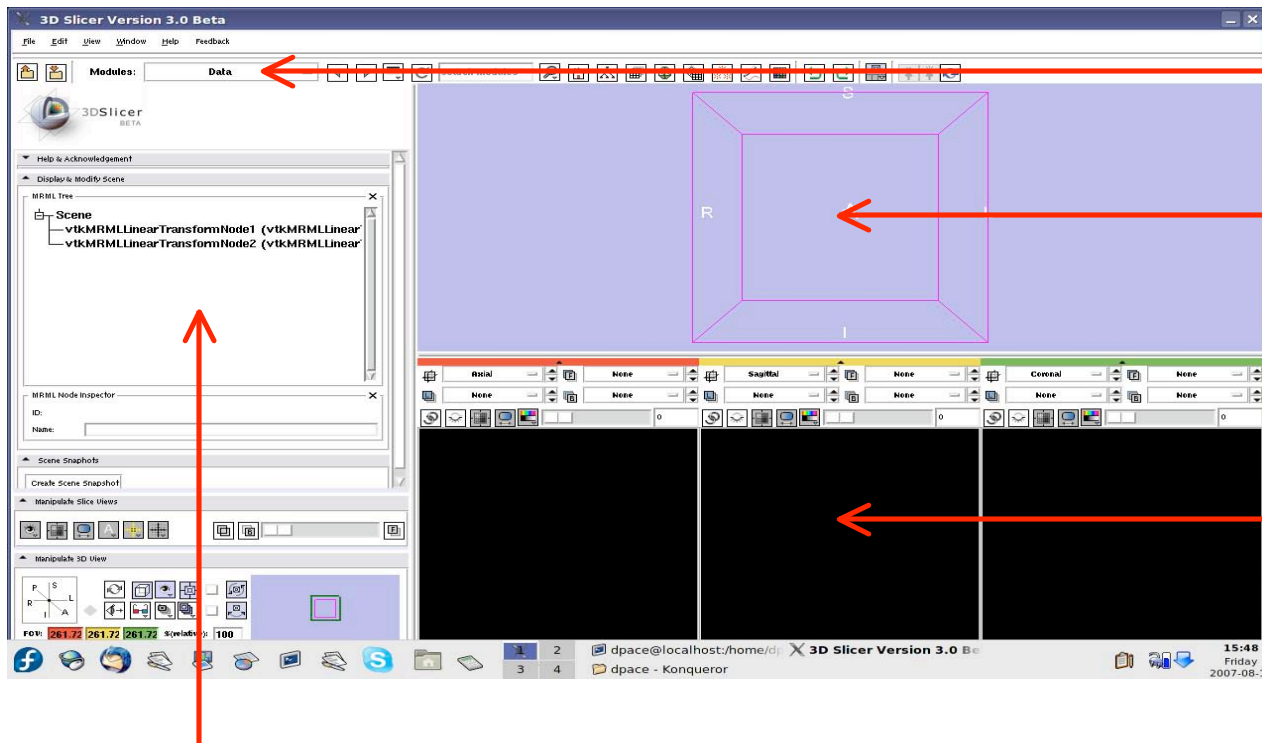

Modules


3D viewer

2D viewer
(axial, sagittal and
coronal views)

Control panes for the current module


2) Load the CT volume

Open the
“Volumes”
module

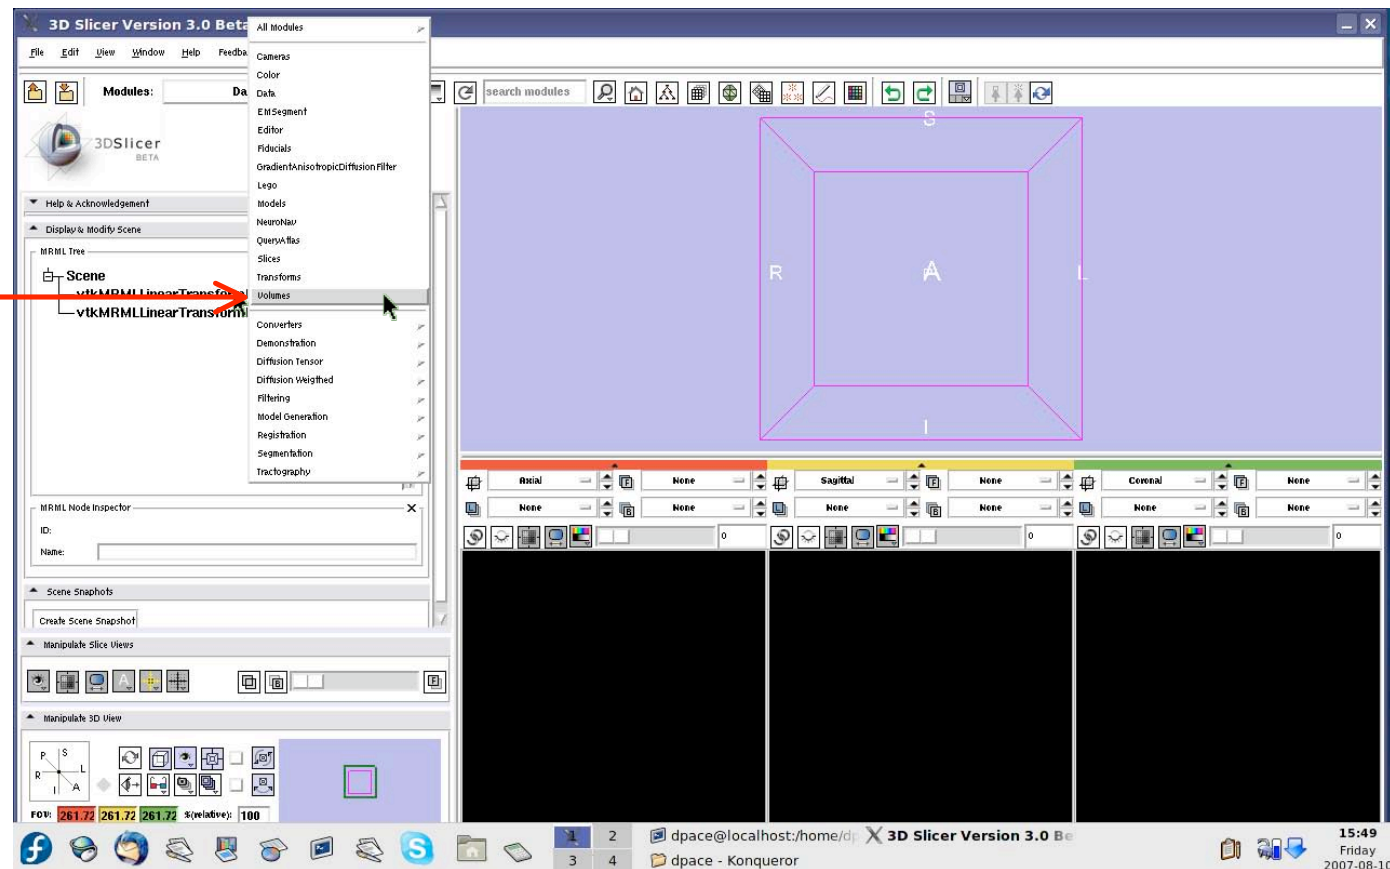


2) Load the CT volume, continued

Click on
"Select
Volume
File"

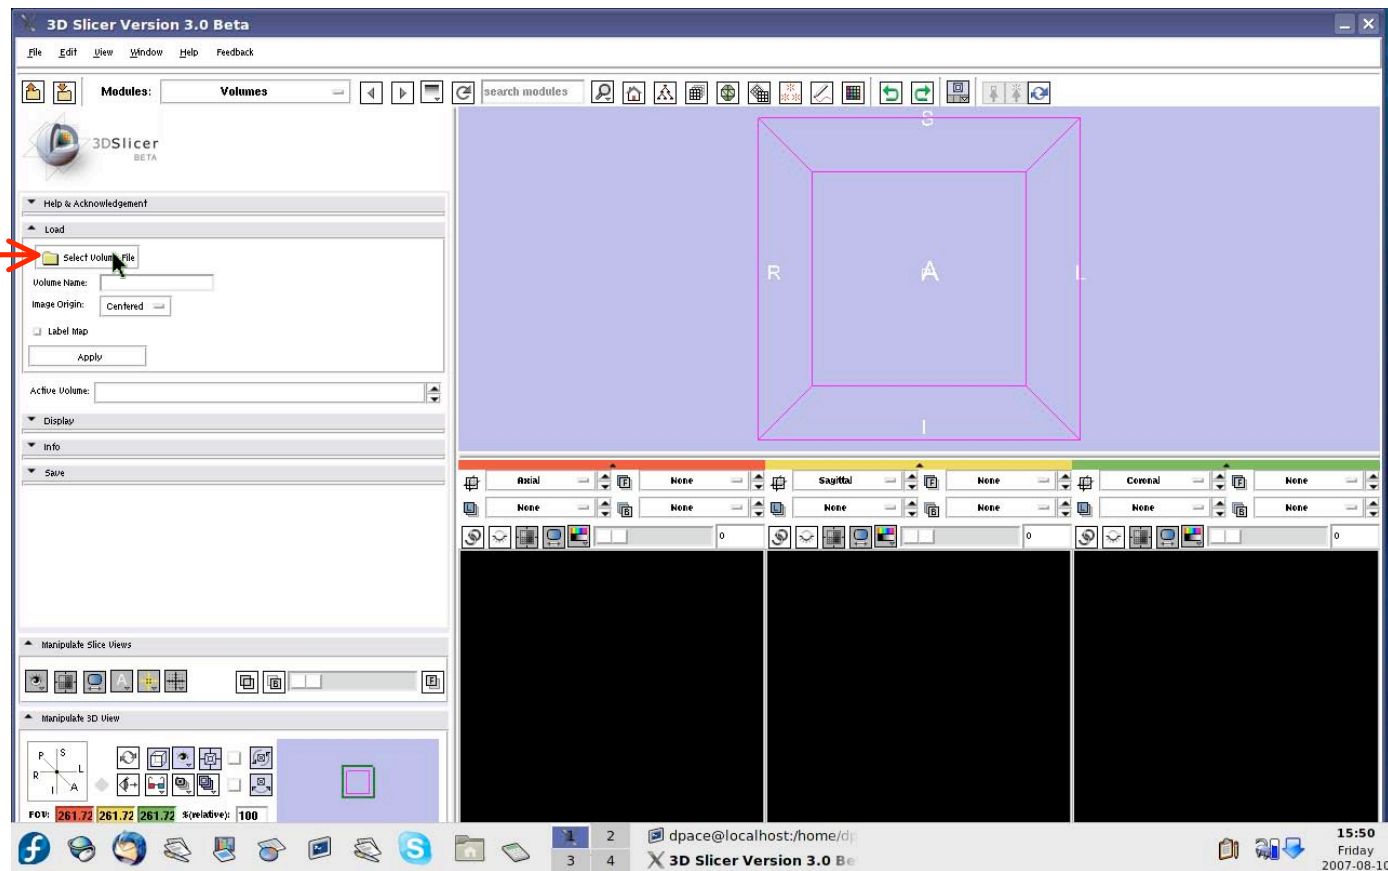


2) Load the CT volume, continued

Click on
the folder
containing
the CT
files, then
click
“Open”

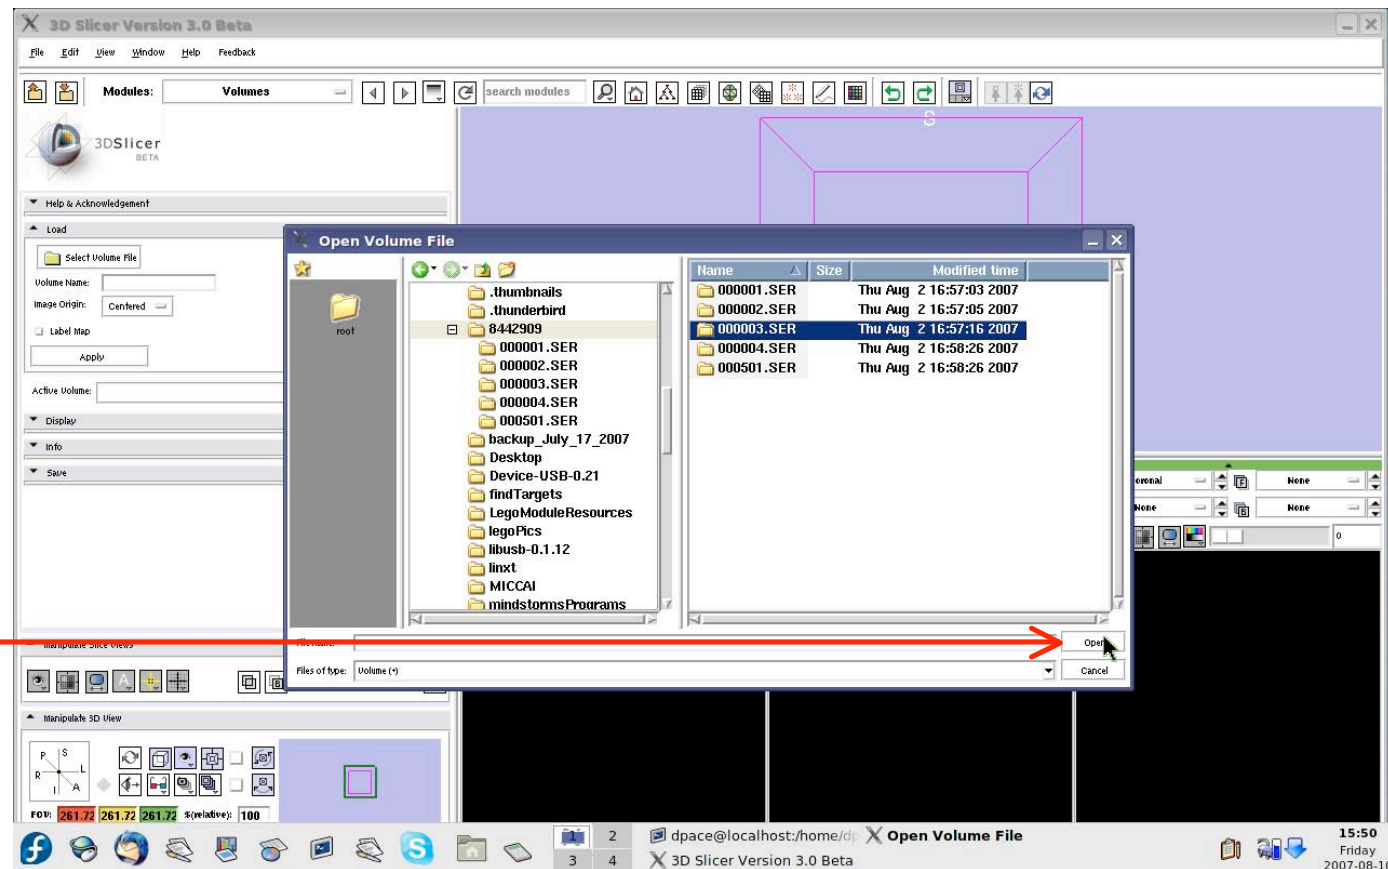


2) Load the CT volume, continued

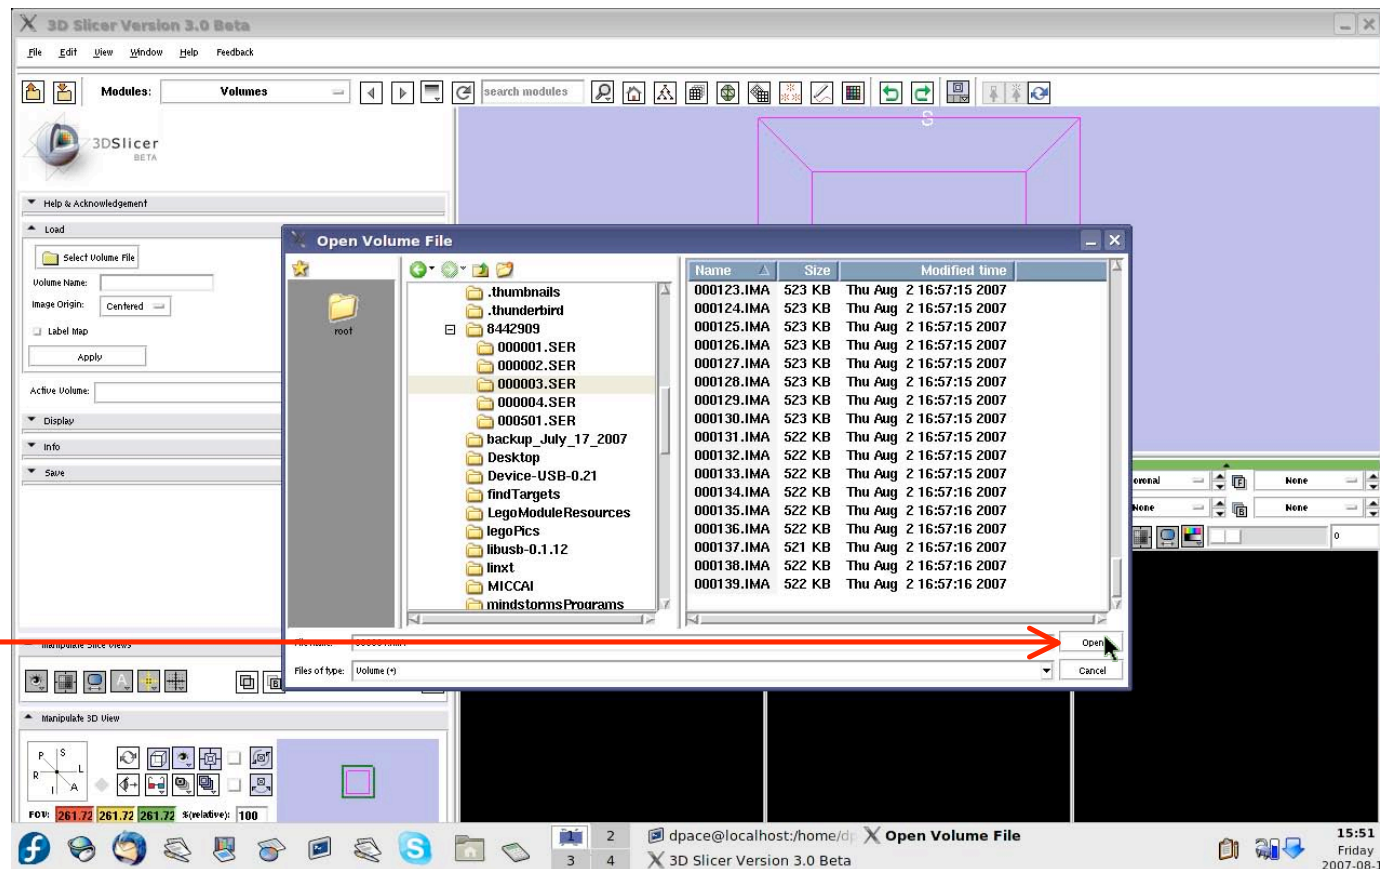


2) Load the CT volume, continued

Click
“Apply”
and wait
until you
see the
CT
volume
in the
viewers

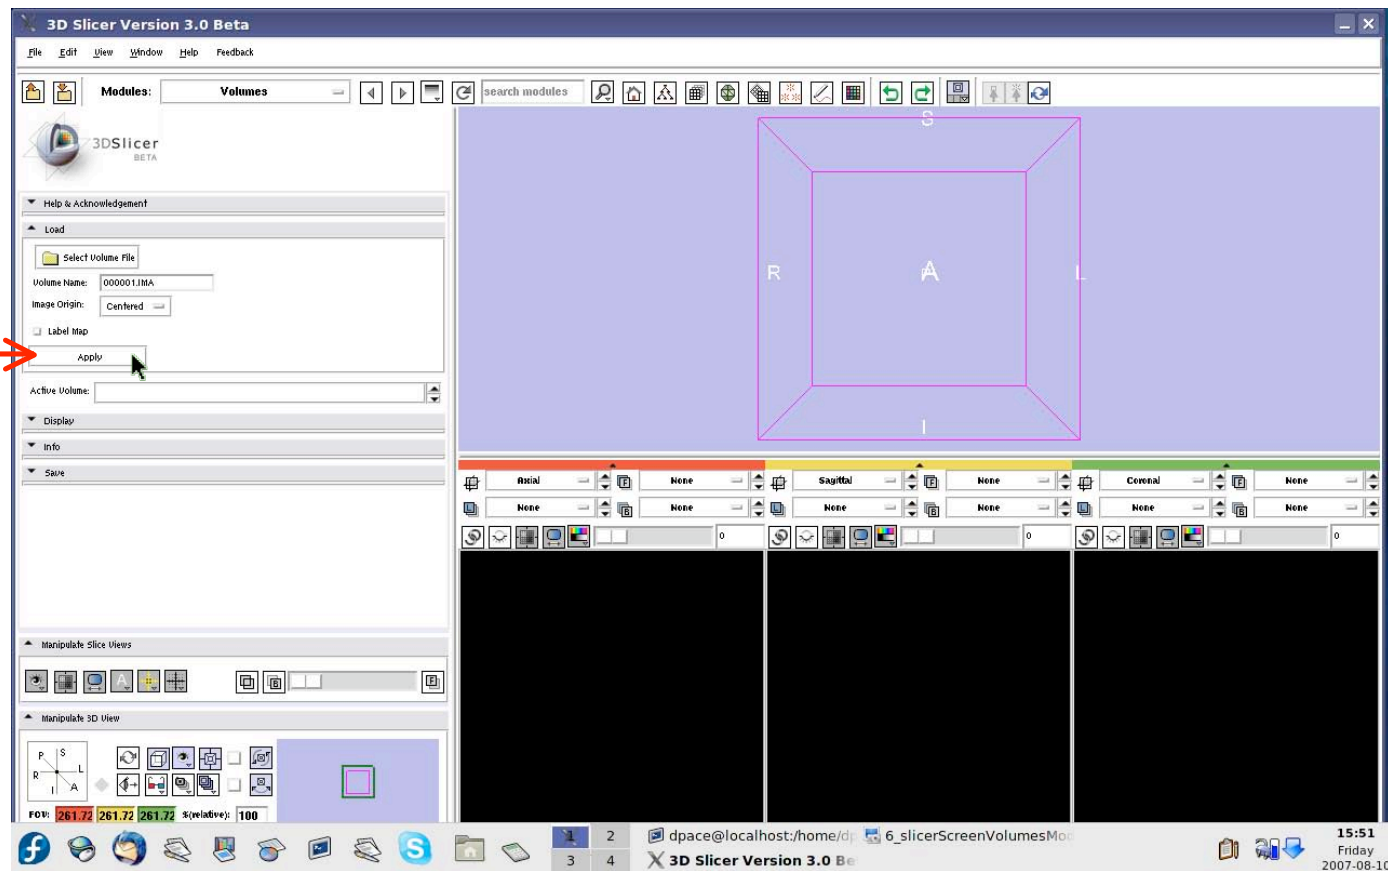

2) Load the CT volume, continued

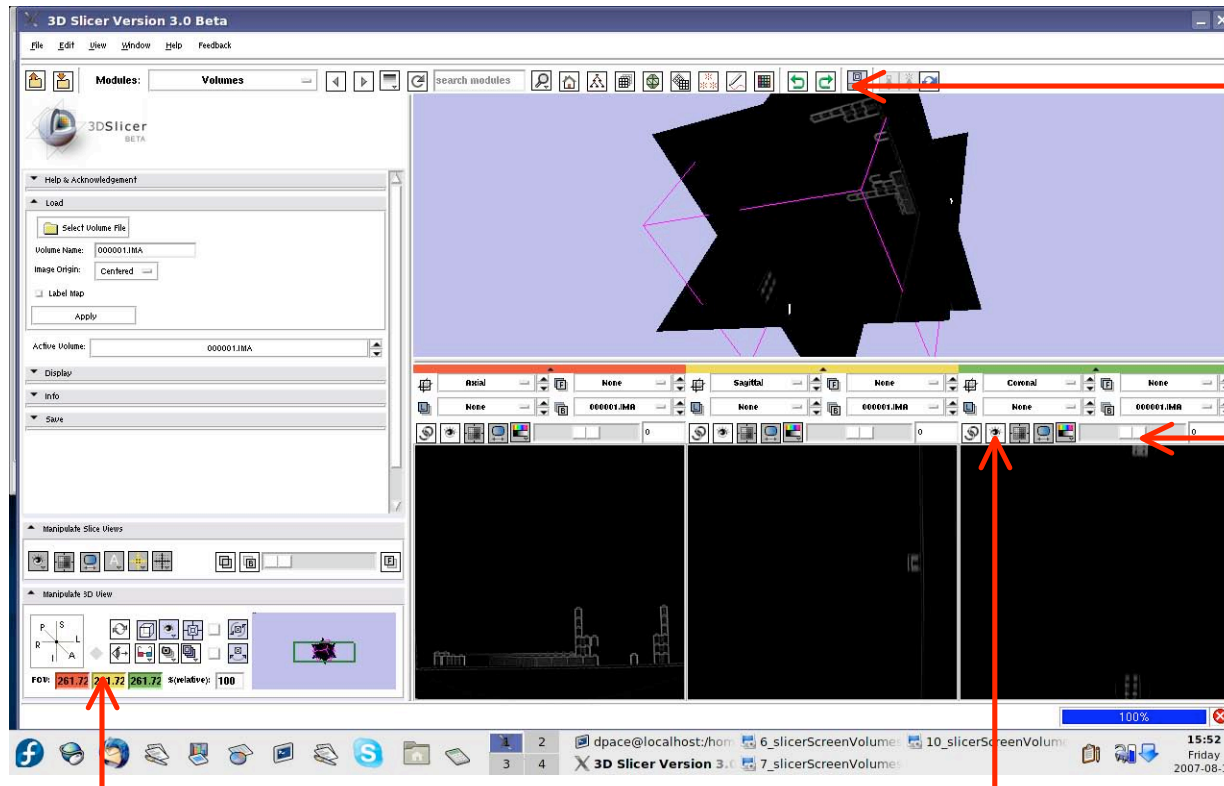

You can click here for different layout options for the viewers


These sliders allow you to scroll through the 2D views of the 3D volume

You can adjust these numbers to change the field of view of the 2D views

You can click here to make the 2D view visible in the 3D viewer


Click on all three of these buttons

2) Load the CT volume, continued

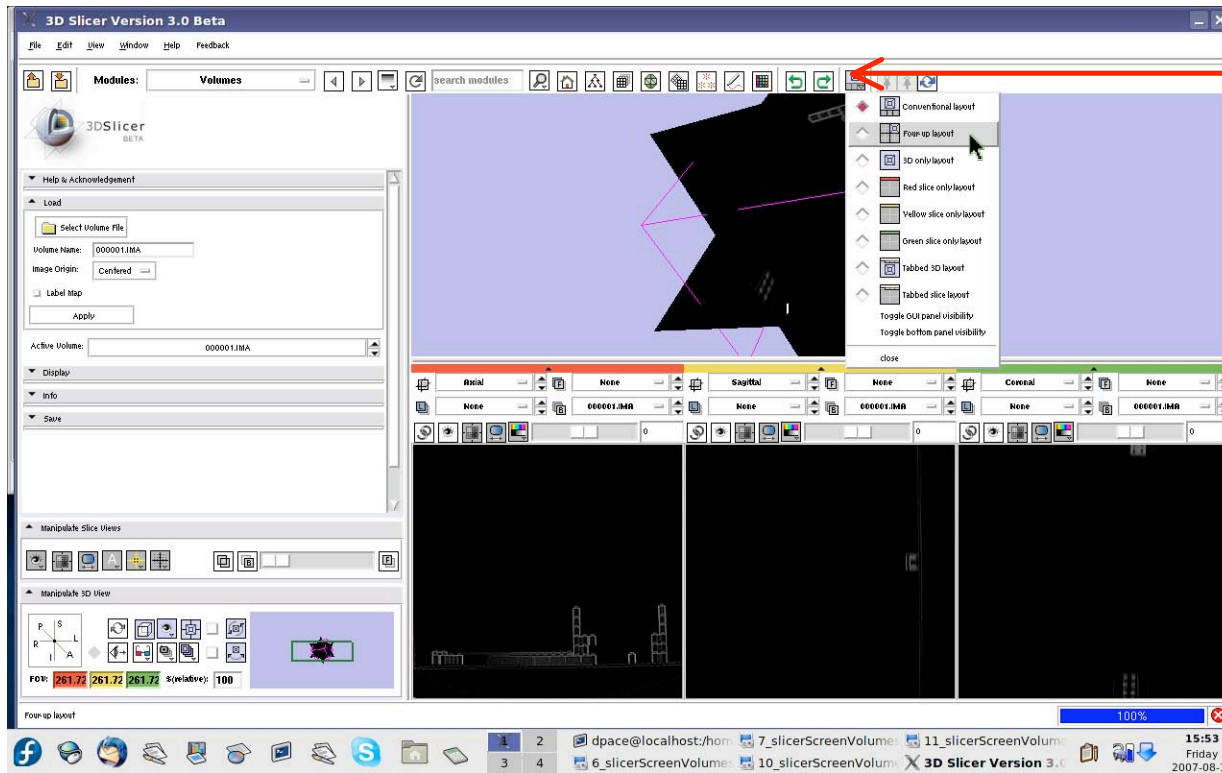

Select the four-up
layout option


2) Load the CT volume, continued

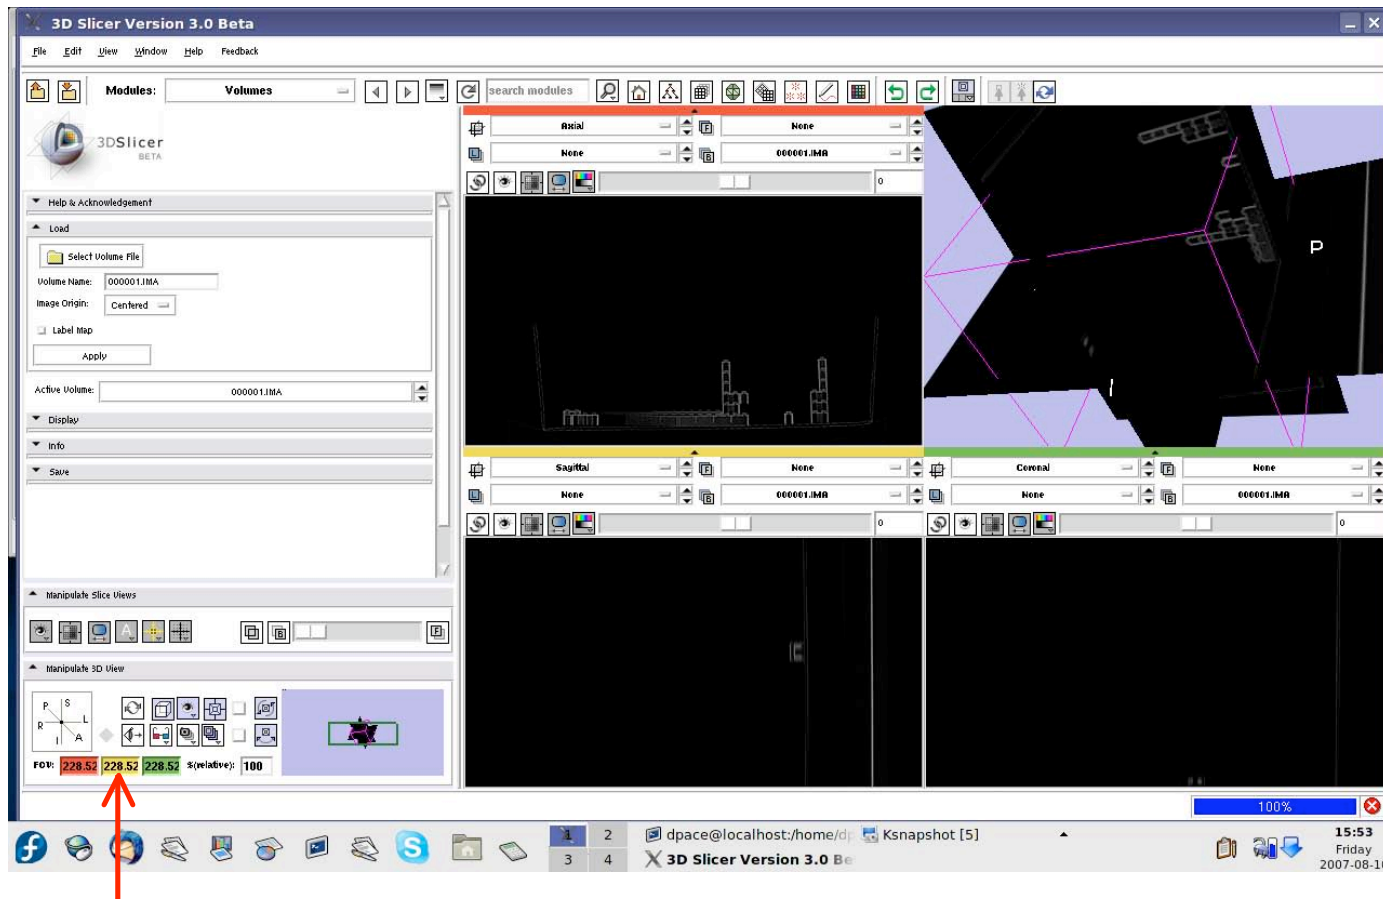

Adjust the field of view for the axial, sagittal and coronal views so that the entire phantom is visible as you scroll through the slices


3) *Connect to the LEGO robot*

Open the "Lego" module

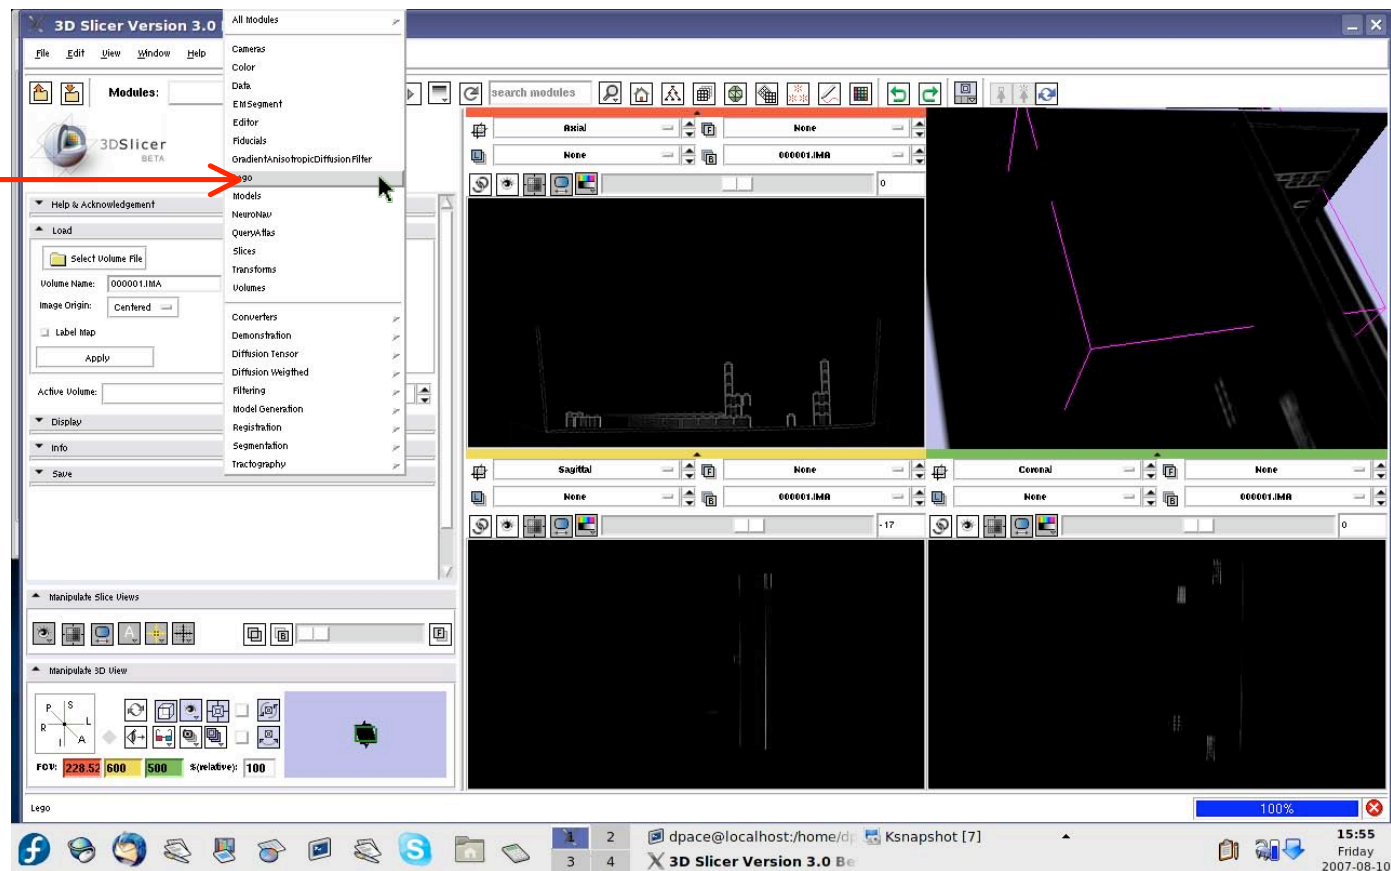


3) Connect to the LEGO robot, continued

Open the "Lego Device" pane

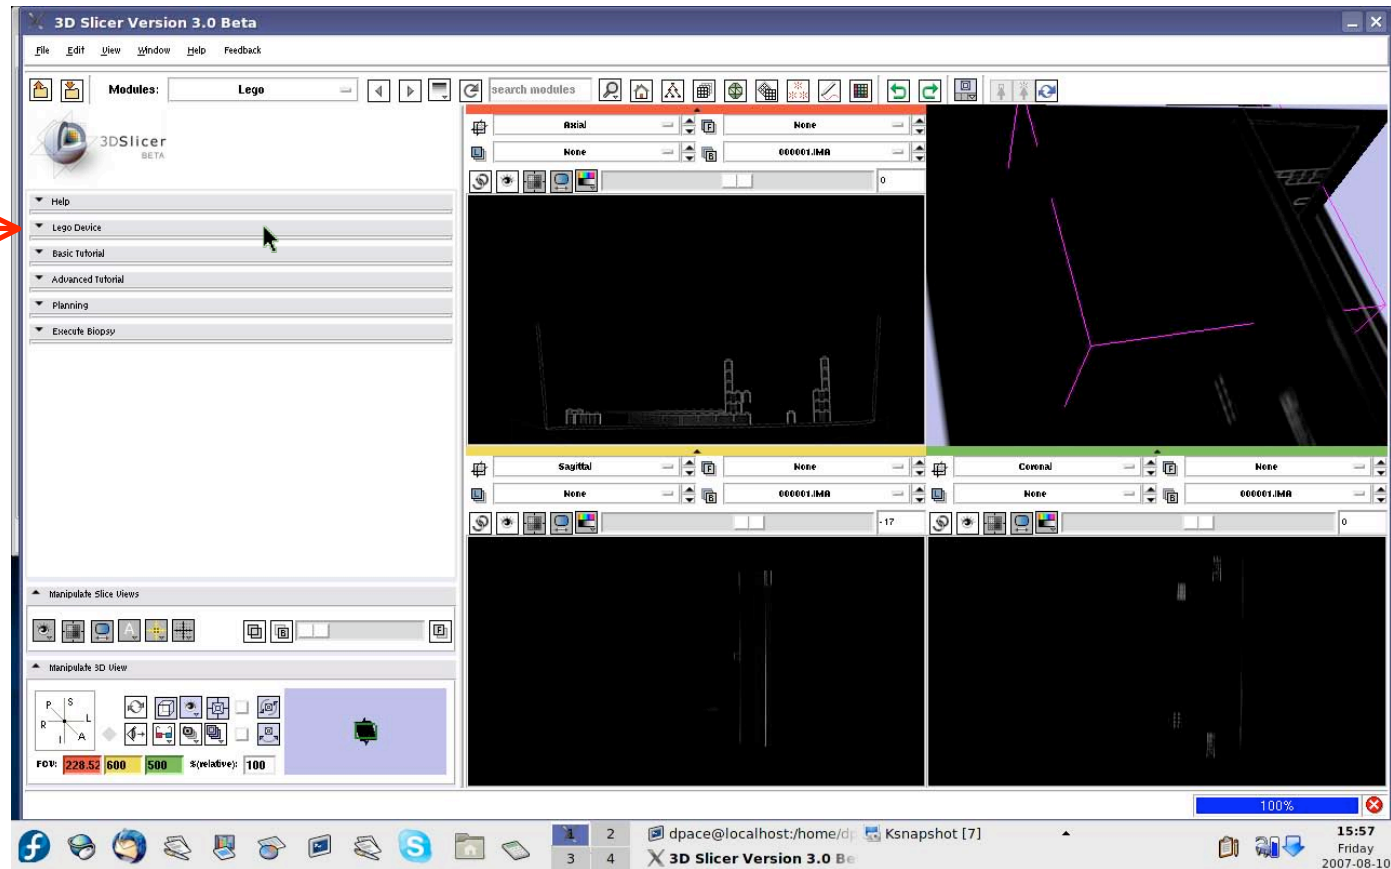


3) Connect to the LEGO robot, continued

Click on the "Connect" check box

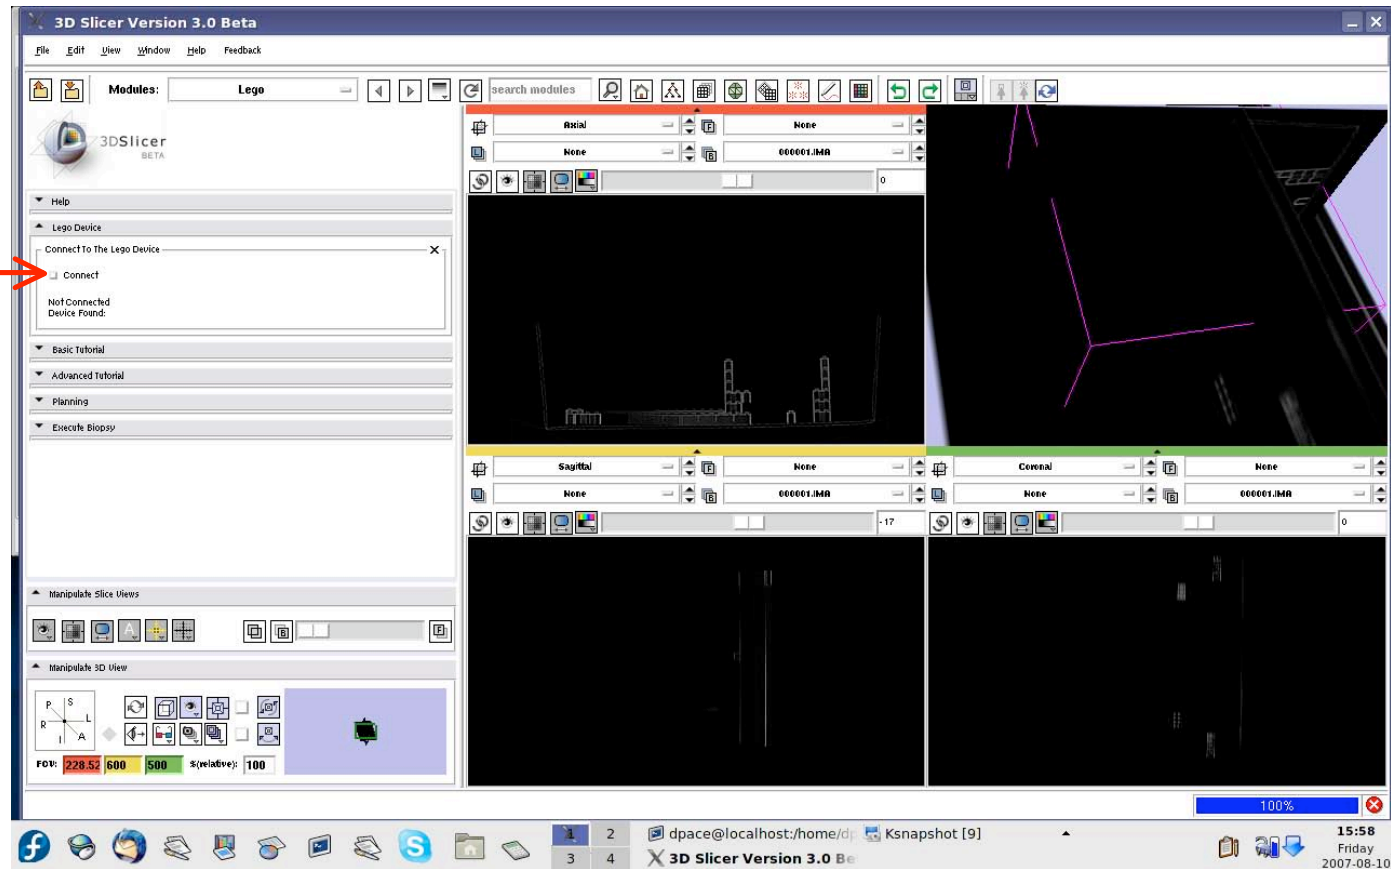

3) Connect to the LEGO robot, continued

Wait until a message appears saying that the connection was successful

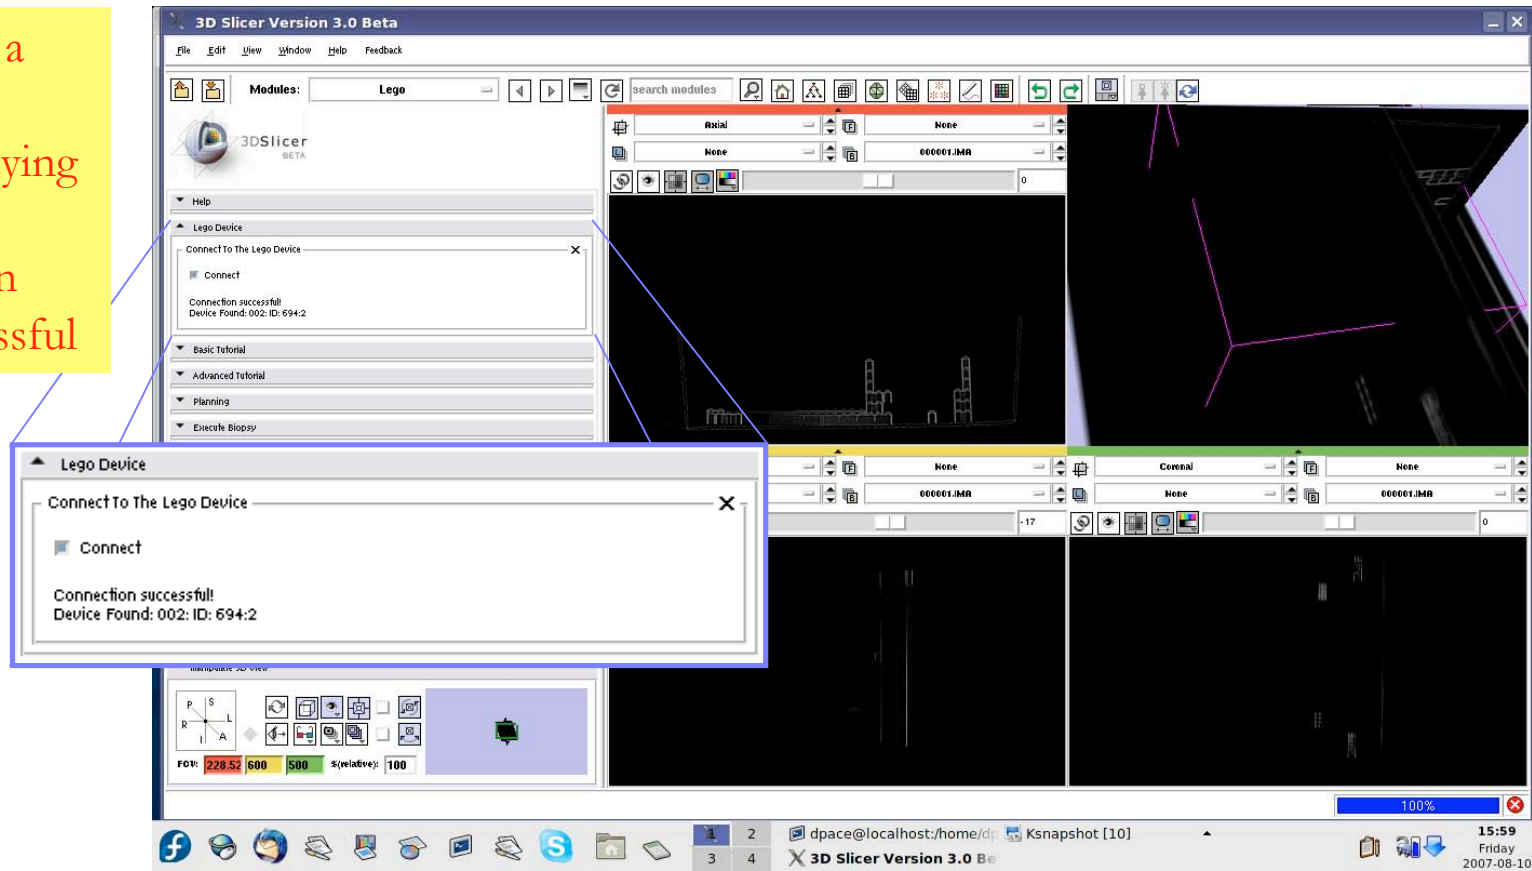


3) Connect to the LEGO robot, continued

- If the connection is not successful, make sure that:
 - You are running as root
 - The LEGO robot is connected to your computer using the USB cable
 - The LEGO robot is turned on


4) *Select the basic tutorial option*

Open the
“Basic
Tutorial”
pane

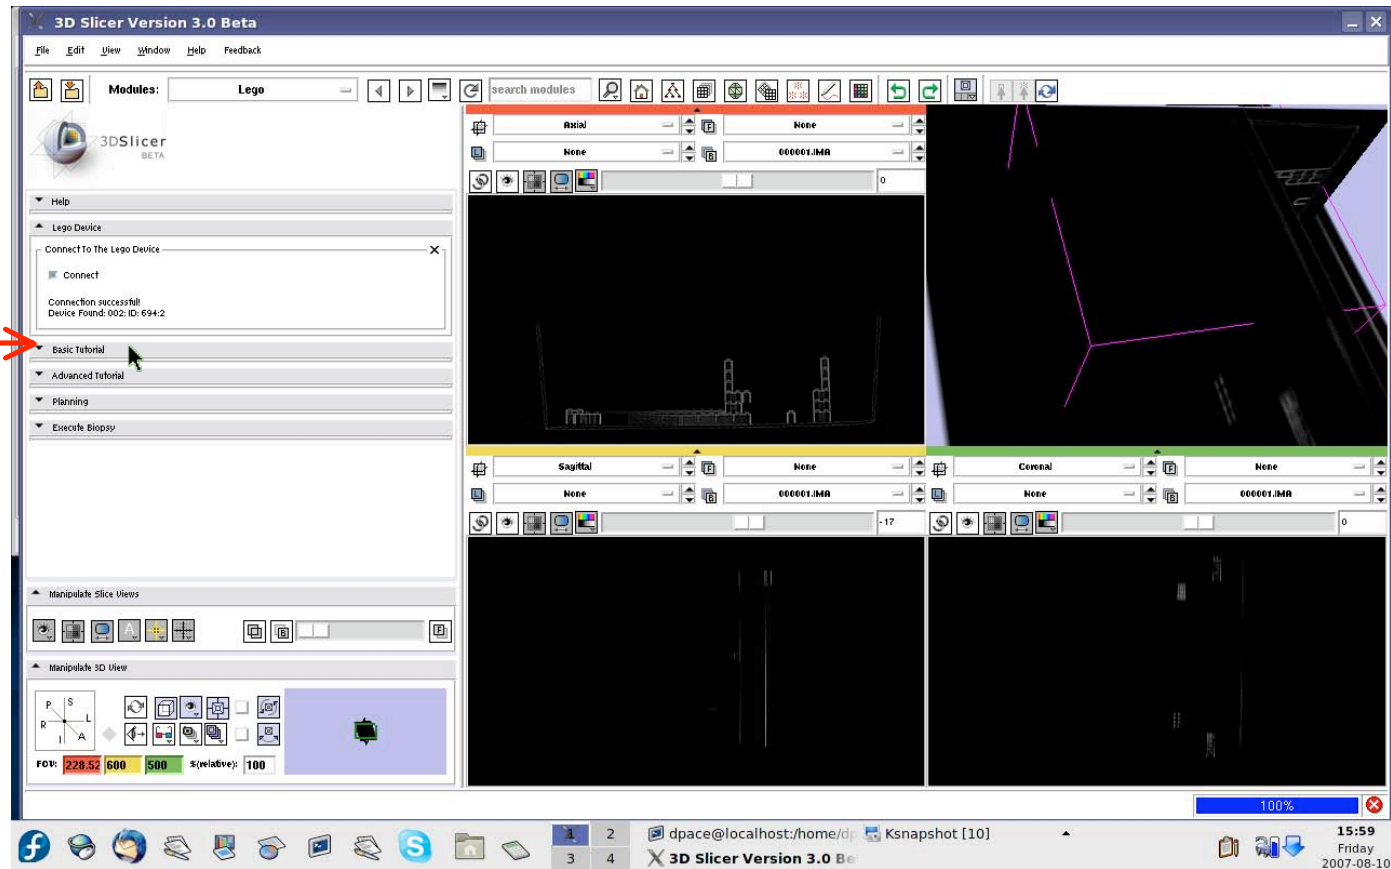


4) *Select the basic tutorial option, continued*

Click on
"Basic
Tutorial"

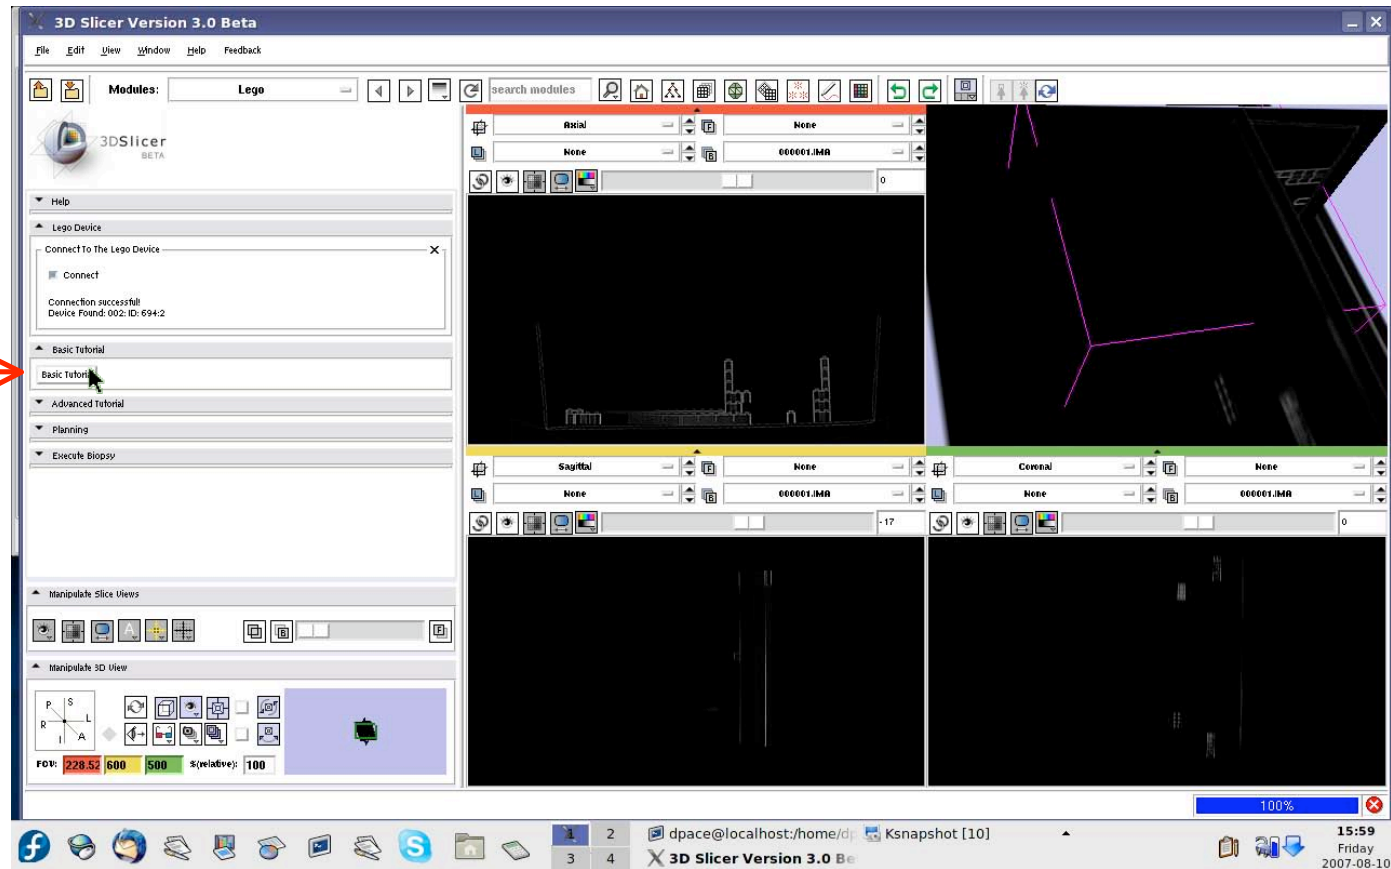


5) *Planning - select the target coordinate*

- The target coordinate is the location where you would like the tip of the robot's needle to be at the end of the “biopsy”.
- Let's try to have the robot biopsy the red pom-pom.
- We need to find the center of the red pom-pom on the CT volume.

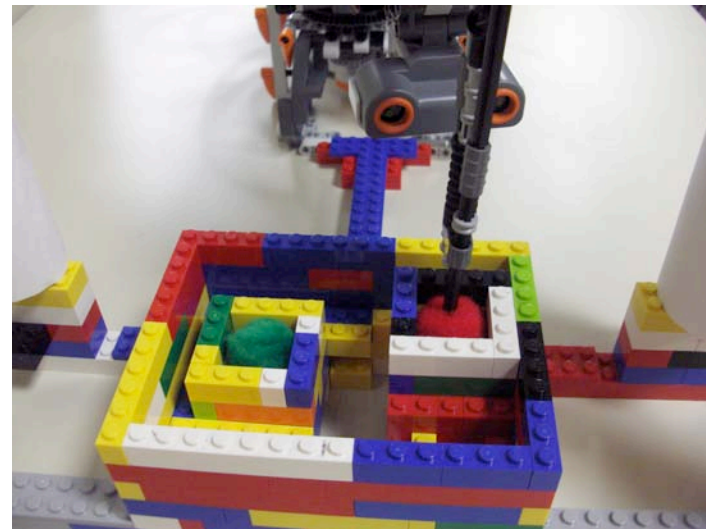


5) Planning - select the target coordinate, continued

Open the
"Planning"
pane

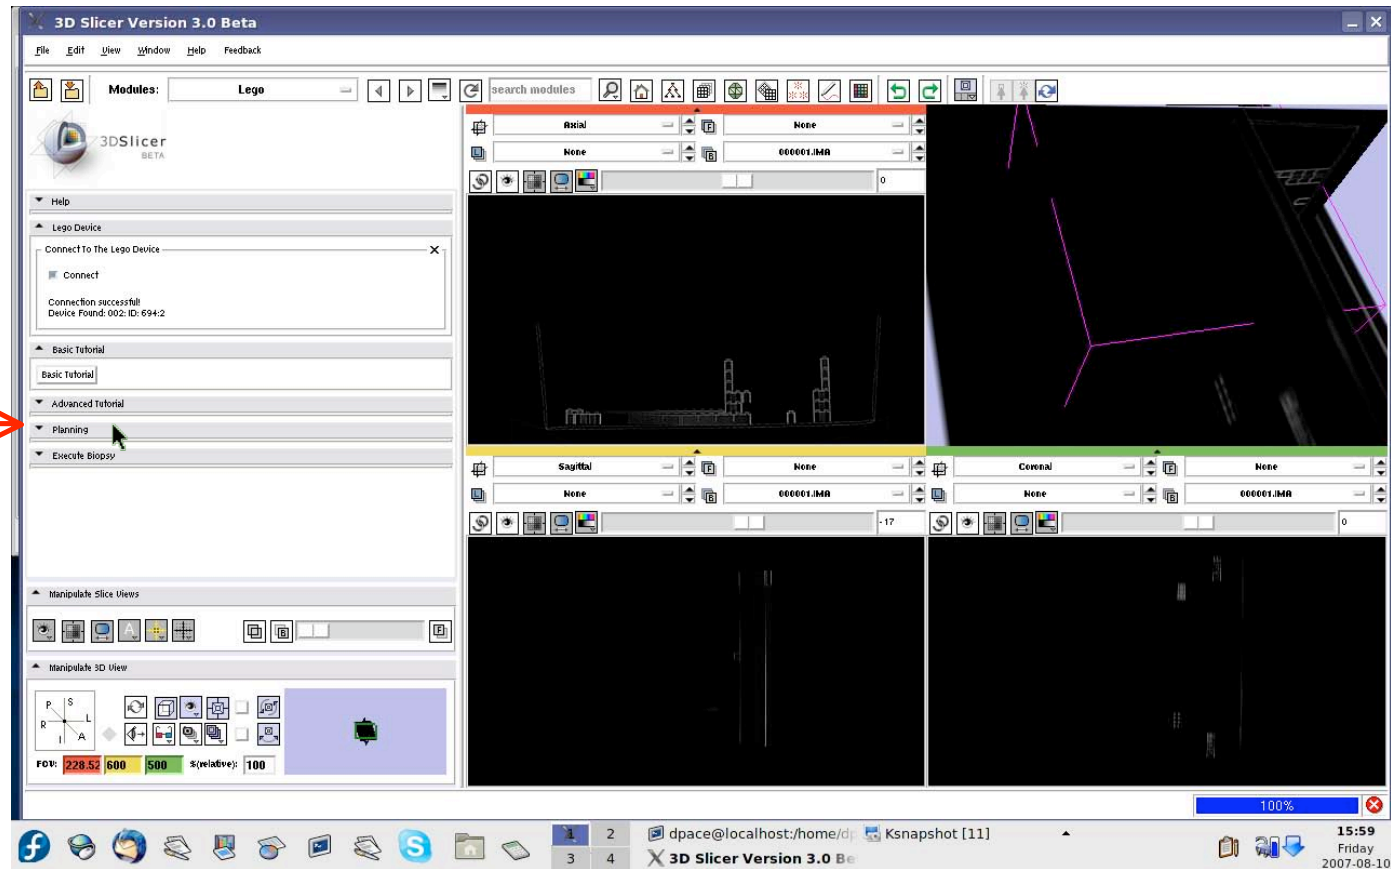

5) Planning - select the target coordinate, continued


Click on
"Target
coordinates"

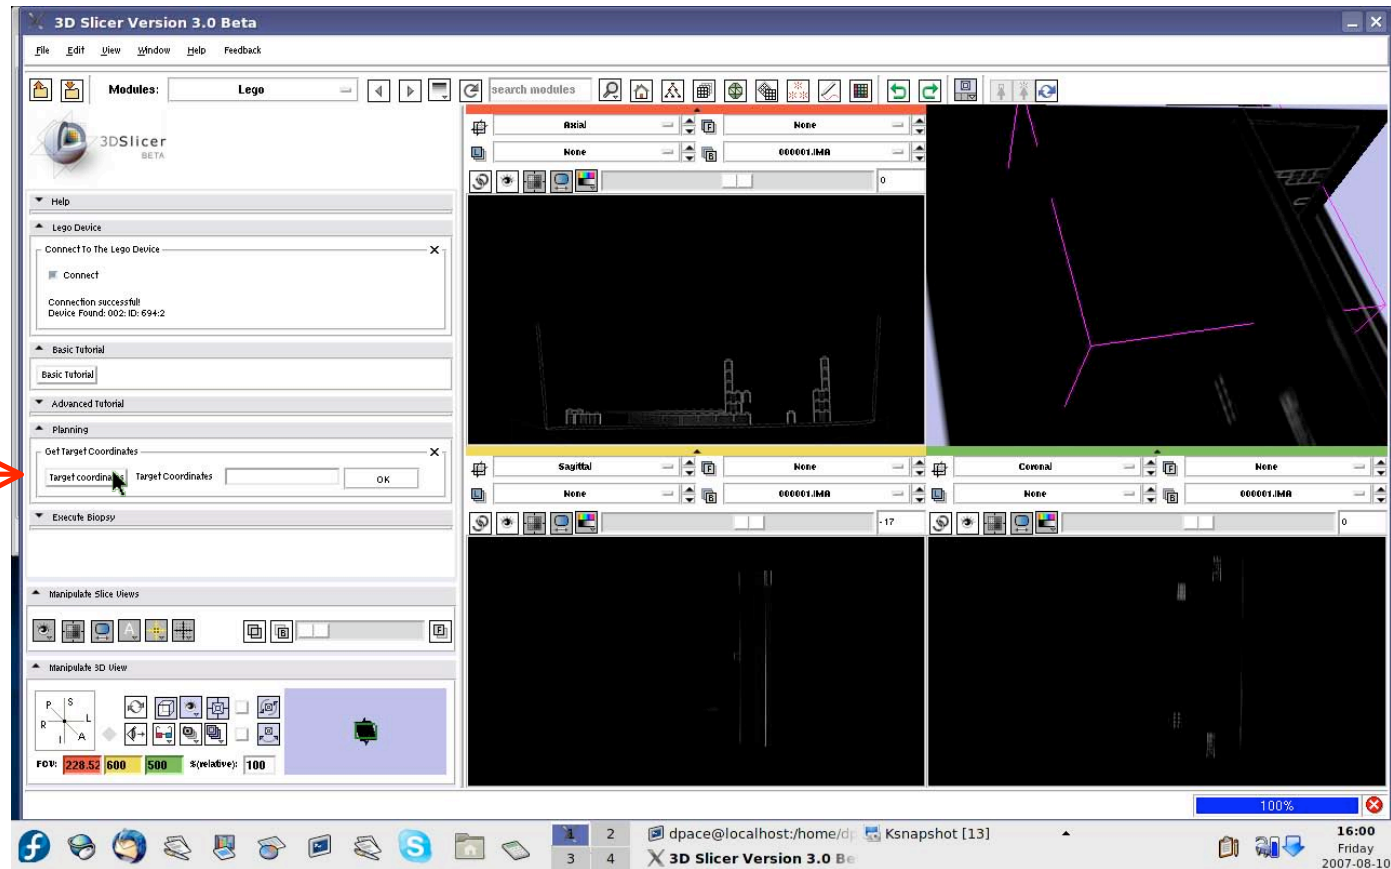

5) Planning - select the target coordinate, continued

Scroll through the 2D viewers using the sliders until you find the center of the red pom-pom. Click on the target coordinate: the center of the red pom-pom.


The area around the current cursor position is shown in more detail here.

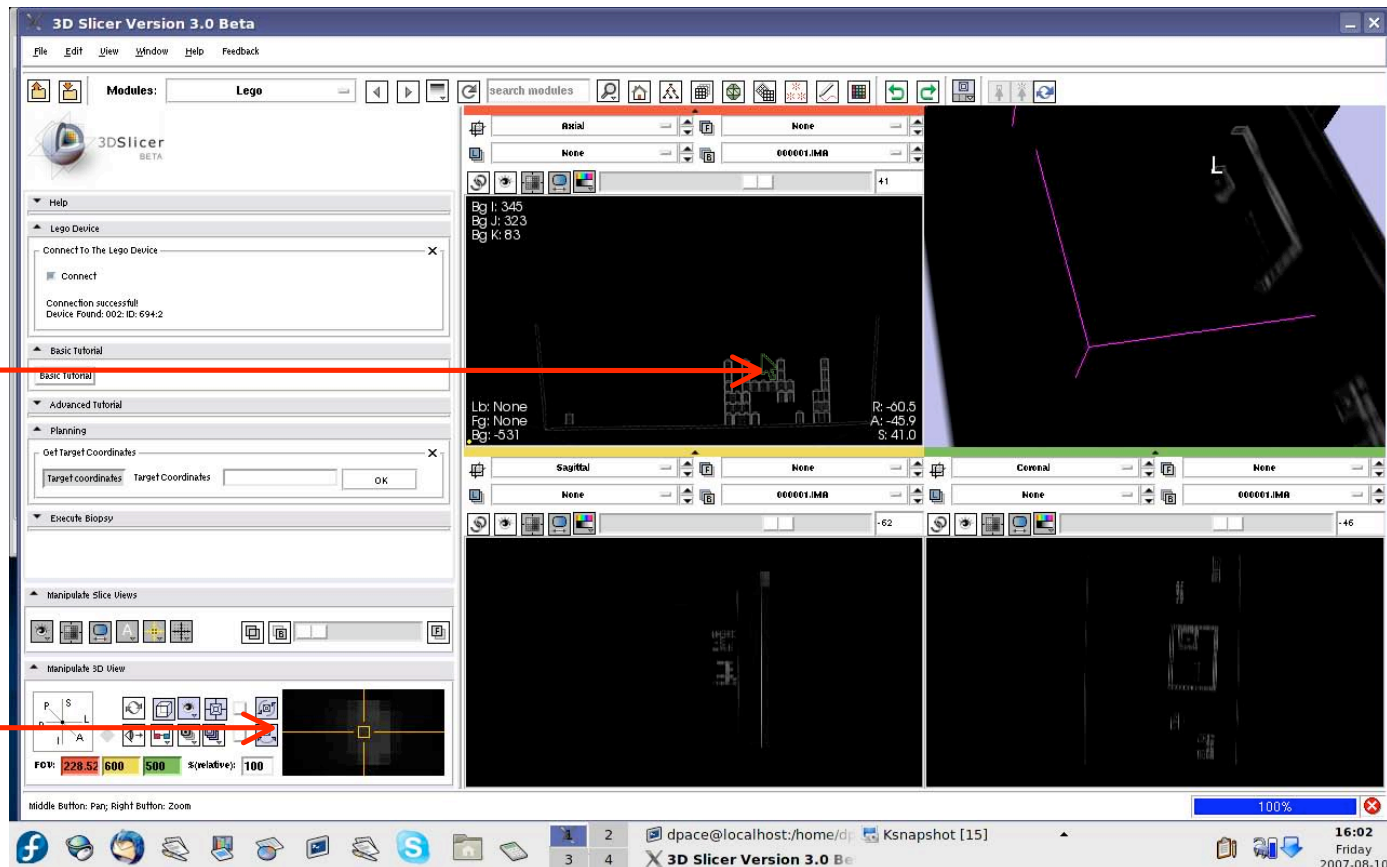

The protrusions on the phantom's pillars will help you orient yourself when scrolling through the CT volume.

5) Planning - select the target coordinate, continued

Click on "OK"
to select the
target coordinate

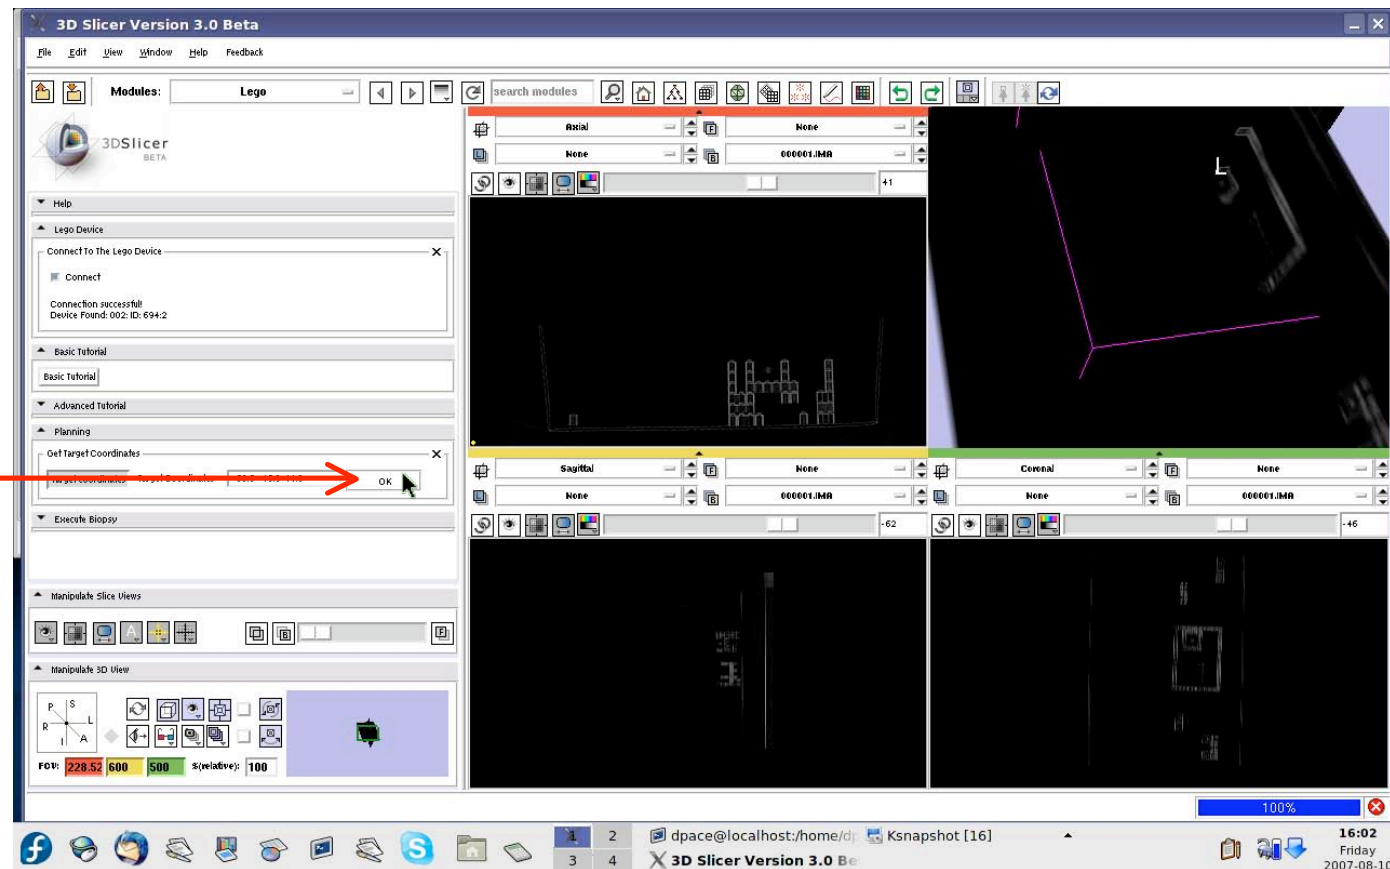


To change the target, click on another point in the CT volume and click on "OK" again.

6) *Execute the biopsy*

Now the
LEGO
robot will
try to hit the
target

Open the
“Execute
Biopsy” pane

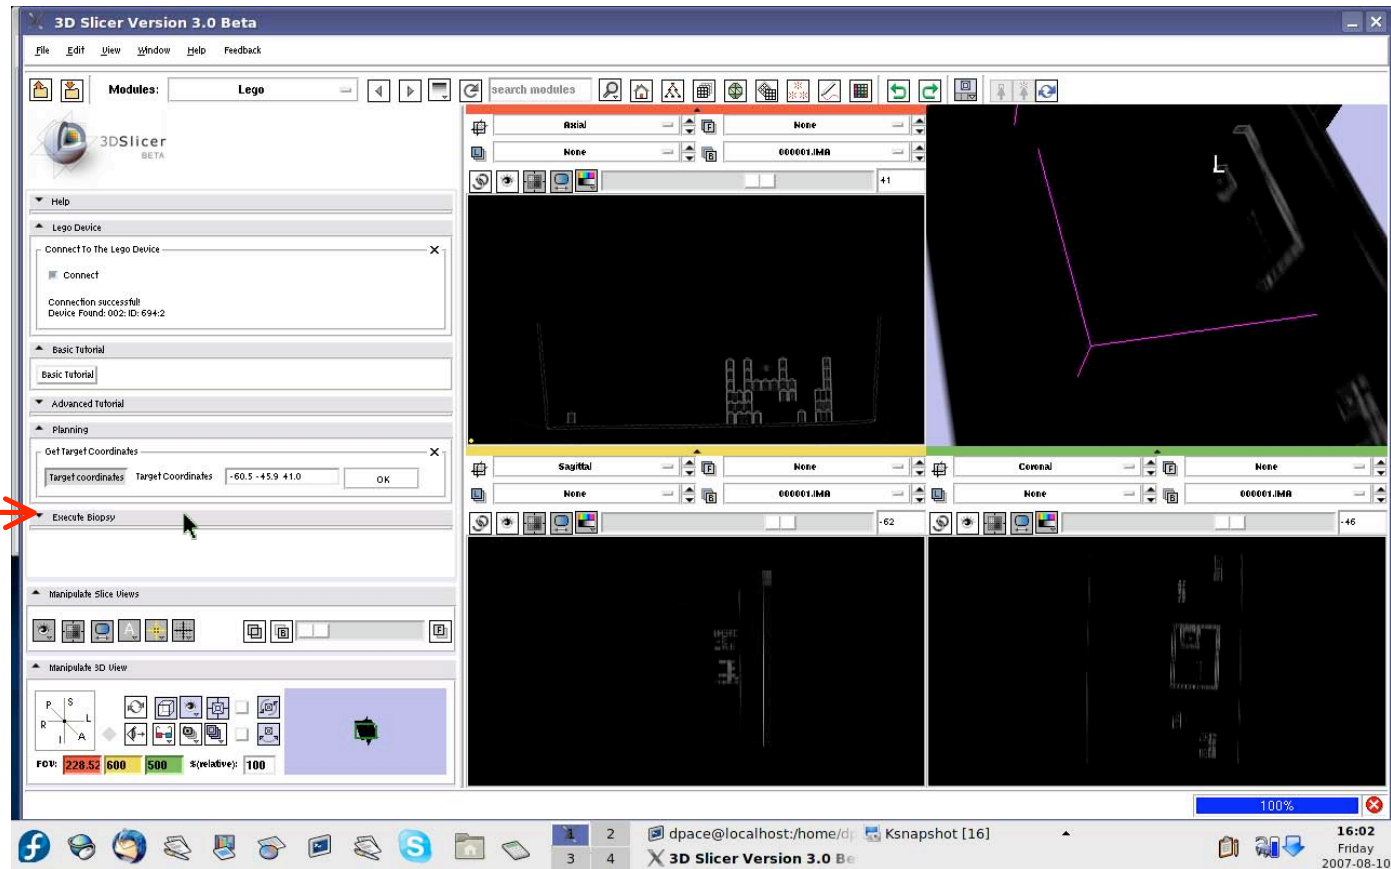


6) Execute the biopsy, continued

Recall:

$$PCS_{3 \times 1} = R_{3 \times 3} \cdot ICS_{3 \times 1} + t_{3 \times 1}$$


The transformation from the image coordinate system to the patient (robot) coordinate system: columns 1-3 show the rotation matrix R ; column 4 shows the translation t .

The target in the image coordinate system that you selected

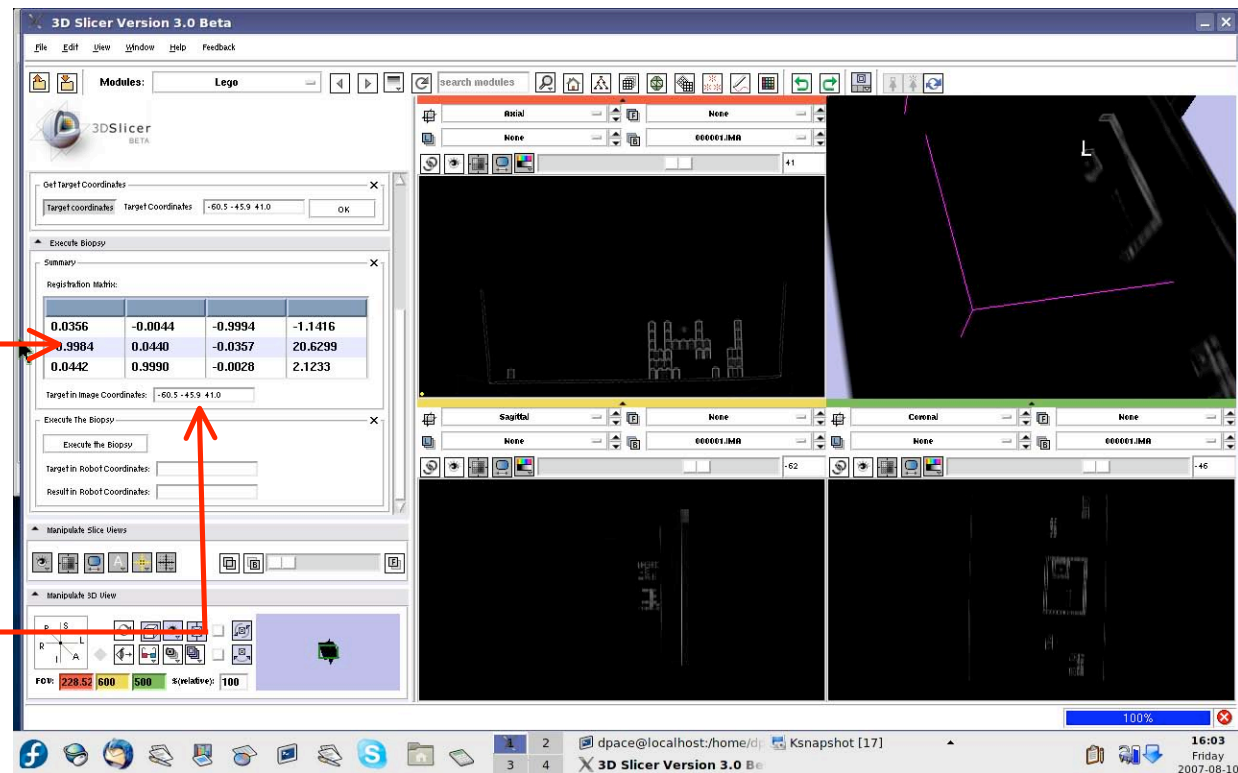


6) *Execute the biopsy, continued*

Click on
“Execute
the Biopsy”

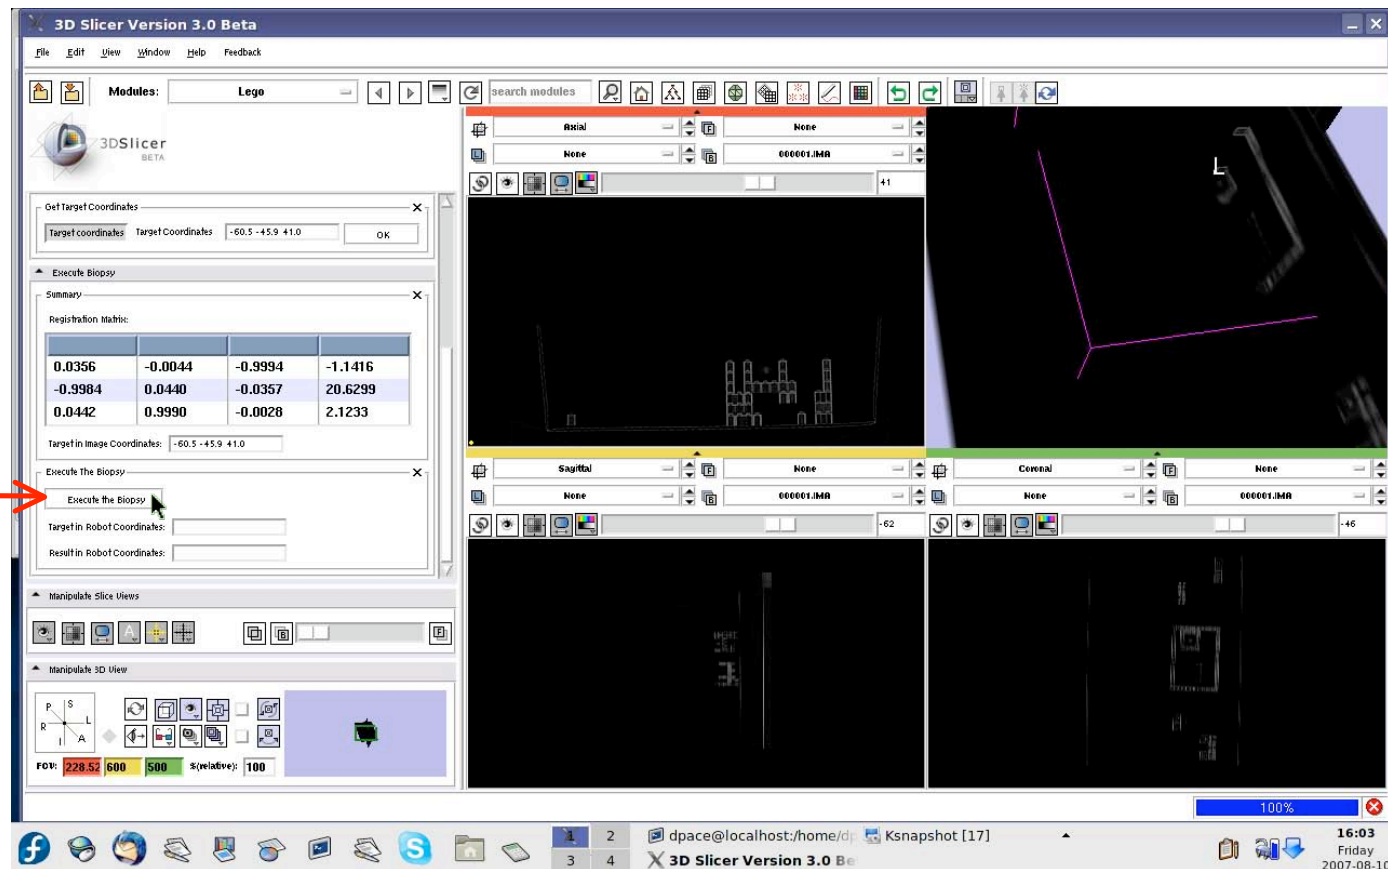


The LEGO
robot will
move to hit
the target!

6) *Execute the biopsy, continued*

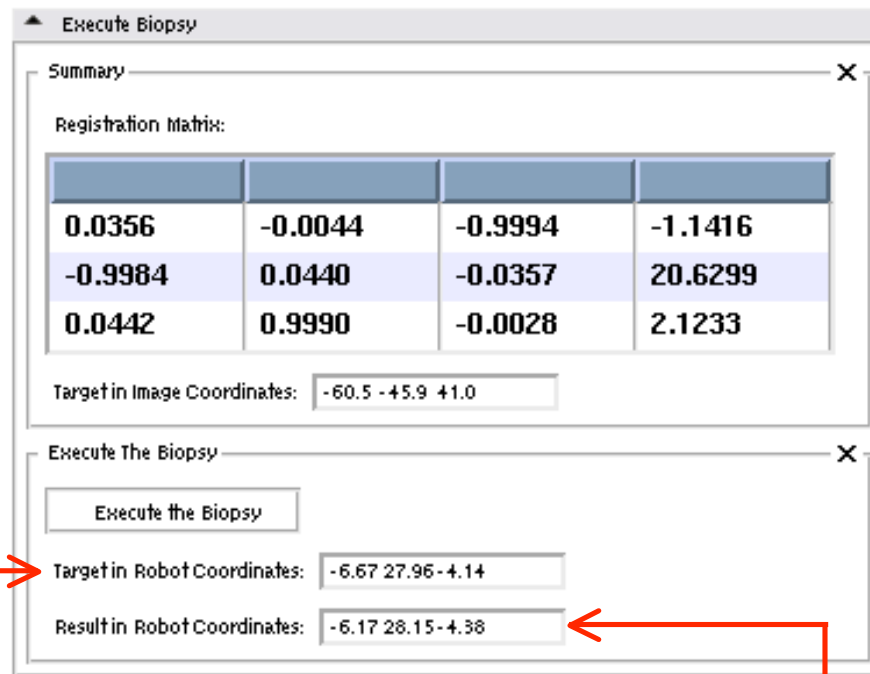

The target in the patient (robot) coordinate system



The final needle position in the patient (robot) coordinate system. This coordinate is calculated using rotational information from the robot's motors and knowledge of the robot's structure, and is not completely accurate.

Tracking is done through targeting during the robot's movement

The display of the final needle position in the *PCS* provides **Navigation**

To select additional targets:

- If you would like to try additional targets, simply go back to the “Planning” pane, select another point on the CT volume and click “OK”. Then go back to the “Execute Biopsy” pane and click “Execute the Biopsy”.

If the LEGO robot does not return to the initial position (centered and all the way back), reset it before selecting another target.

After completing this tutorial section

- You have learned about the following steps in IGT and medical robotics in a hands-on manner:
 - ✓ Imaging
 - ✓ Preoperative planning
 - ✓ Targeting and tracking
 - ✓ Navigation

Thanks to

- Terry Peters, Ph.D, (Robarts Research Institute, University of Western Ontario)
- Steven Canvin (The LEGO Group)
- Cory Walker (NXT++ Developer)
- G. Wade Johnson (Device::USB Developer)
- Steve Pieper, Ph.D (Surgical Planning Laboratory)
- Haiying Liu (Surgical Planning Laboratory)
- Junichi Tokuda, Ph.D (Surgical Planning Laboratory)
- Christoph Ruetz (Surgical Planning Laboratory)
- Philip Mewes (Surgical Planning Laboratory)
- The entire LEGO Mindstorms community